

Knobbe Martens Olson & Bear LLP

Intellectual Property Law



10/020002

Cap C \$
2040 Main Street
Fourteenth Floor
Irvine, CA 92614
Tel 949-760-0404
Fax 949-760-9502
www.kmob.com

Mark J. Kertz

September 29, 2005

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

Certificate
OCT 07 2005
of Correction

Re: METHOD OF IMPLANTING AN INTRAOCULAR
LENS SYSTEM

Letters Patent No. 6,899,732

Issued: May 31, 2005

Our Reference: VGEN.010A

Dear Sir:

Enclosed for filing is a Certificate of Correction in connection with the above-identified patent.

As the error cited in the Certificate of Correction was incurred through no fault of the Patent Office, enclosed is our check in the amount of \$100. Please charge any additional fees to our Deposit Account No. 11-1410.

An explanation of the error and the corrections is set forth below.

Figures 18 and 19 are described at Column 15, line 60 to Column 16, line 45. Figures 18 and 19 are depicted below:

10/04/2005 AKELECH1 00000014 6899732

01 FC:1811

100.00 DP

OCT 12 2005

San Diego
619-235-8550

San Francisco
415-954-4114

Los Angeles
310-551-3450

Riverside
951-781-9231

San Luis Obispo
805-547-5580

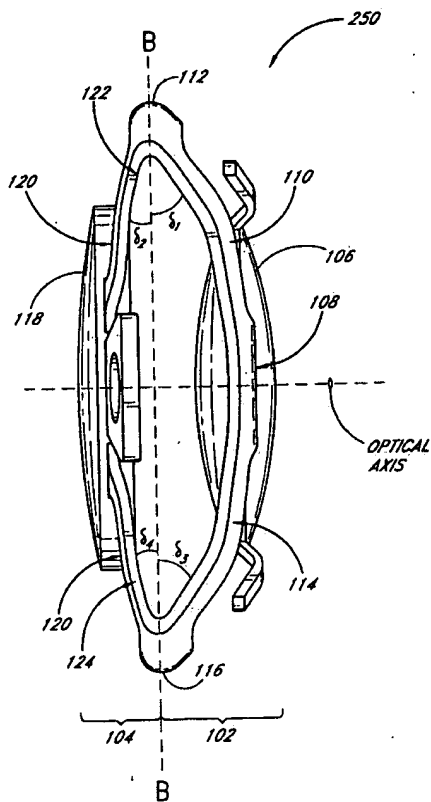


FIG. 18

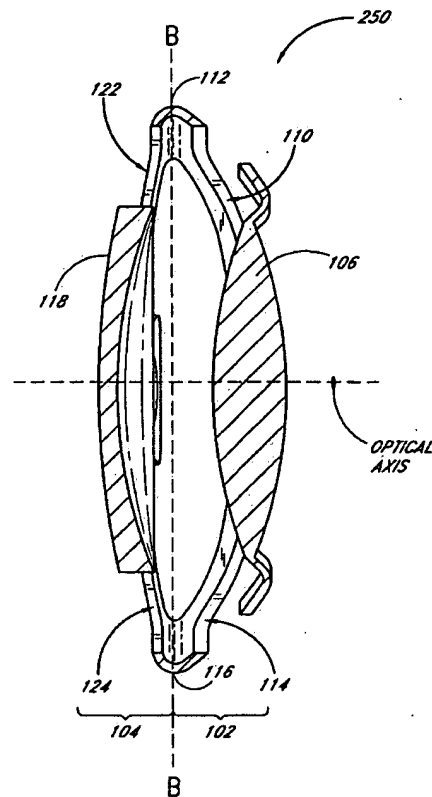


FIG. 19

The textual descriptions of Figures 18 and 19 contain a minor, obvious error at Column 16, line 12, in that the angles shown at the bottom of the lens system of Figures 18 and 19 are described as being substantially equal. Obviously, they are not. Indeed, the remainder of the description makes it abundantly clear that what is being described is a lens having asymmetry as viewed from the side, and that is exactly what the Figures depict. The correction to the specification made in the enclosed Certificate of Correction properly describes the angles as being unequal, and makes line 12 consistent with the other 53 lines of text that describe Figures 18 and 19, as well as with the figures themselves.

Respectfully submitted,

Knobbe, Martens, Olson & Bear, LLP

Mark Kert

Mark J. Kertz
Registration No. 43,711
Customer No. 20,995

Enclosures

UNITED STATES PATENT AND TRADEMARK OFFICE

CERTIFICATE OF CORRECTION

PATENT NO. : 6,899,732

DATED : May 31, 2005

INVENTOR(S): Gholam Zadno-Azizi, et al.

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the specification, Col. 16, Line 12, delete "substantially equal" and substitute --unequal--.

MAILING ADDRESS OF SENDER:

Mark J. Kertz
KNOBBE, MARTENS, OLSON & BEAR, LLP
2040 Main Street, 14th Floor
Irvine, California 92614

PATENT NO. 6,899,732